


Dilation

CRE™ CONTROLLED RADIAL EXPANSION DILATION BALLOONS



NEW CRE™ Wire-guided Esophageal/Pyloric/Biliary Dilation Balloons (including DASE indication)†

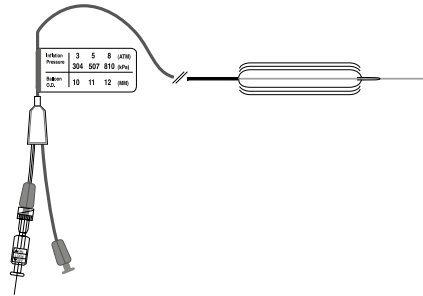

Order Number	Inflated O.D. (mm)	Balloon Length (cm)	Inflation Pressure		Minimum Working Channel (mm)	Catheter Diameter (F) / (mm)	Working Length (cm)
			(ATM)	(kPa)			
M00558600	6-7-8	5.5	3-6-10	304-608-1013	2.8 (A)/3.2 (B)	7.5 / 2.50	180
M00558610	8-9-10	5.5	3-5-5-9	304-557-912	2.8 (A)/3.2 (B)	7.5 / 2.50	180
M00558620	10-11-12	5.5	3-5-8	304-507-811	2.8 (A)/3.2 (B)	7.5 / 2.50	180
M00558630	12-13.5-15	5.5	3-4-5-8	304-456-811	2.8 (A)/3.2 (B)	7.5 / 2.50	180
M00558640	15-16.5-18	5.5	3-4-5-7	304-456-709	2.8/3.2 (A)/4.2 (B)*	7.5 / 2.50	180
M00558650	18-19-20	5.5	3-4-5-6	304-456-608	2.8/3.2 (A)/4.2 (B)*	7.5 / 2.50	180

Packaged one per box

Recommended Inflation Device: Alliance II Integrated Inflation System Re-usable Handle M00550620, Sterile Syringe M00550601

Pre-assembled .035in (0.89mm) Guidewire


(A) = Alimentary tract

(B) = Biliary tract

* Requires a 2.8mm Olympus Endoscope channel or a 3.2mm Pentax or Fujinon Endoscope channel for alimentary tract.

† Product available in the European Economic Area (EEA) only. Please check availability of the product with your local sales representative or your local customer service.

This product contains no detectable latex.

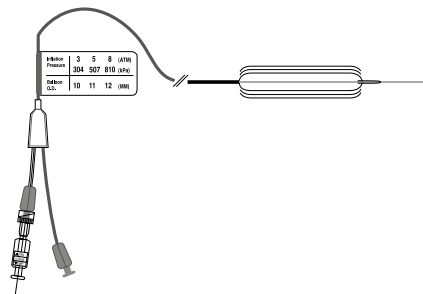

NEW CRE™ Wire-guided Esophageal/Pyloric/Colonic/Biliary Dilation Balloons (including DASE indication)†



Order Number	Inflated O.D. (mm)	Balloon Length (cm)	Inflation Pressure		Minimum Working Channel (mm)	Catheter Diameter (F) / (mm)	Working Length (cm)
			(ATM)	(kPa)			
M00558660	6-7-8	5.5	3-6-10	304-608-1013	2.8/3.2 (A)/3.2 (B)*	7.5 / 2.50	240
M00558670	8-9-10	5.5	3-5-5-9	304-557-912	2.8/3.2 (A)/3.2 (B)**	7.5 / 2.50	240
M00558680	10-11-12	5.5	3-5-8	304-507-811	2.8/3.2 (A)/3.2 (B)*	7.5 / 2.50	240
M00558690	12-13.5-15	5.5	3-4-5-8	304-456-811	2.8/3.2 (A)/3.2 (B)*	7.5 / 2.50	240
M00558700	15-16.5-18	5.5	3-4-5-7	304-456-709	2.8/3.2 (A)/3.2 (B)*	7.5 / 2.50	240
M00558710	18-19-20	5.5	3-4-5-6	304-456-608	2.8/3.2 (A)/3.2 (B)*	7.5 / 2.50	240

Packaged one per box

Recommended Inflation Device: Alliance II Integrated Inflation System Re-usable Handle M00550620, Sterile Syringe M00550601

Pre-assembled .035in (0.89mm) Guidewire


(A) = Alimentary tract

(B) = Biliary tract

* Requires a 2.8mm Olympus Endoscope channel or a 3.2mm Pentax or Fujinon Endoscope channel for alimentary tract.


† Product available in the European Economic Area (EEA) only. Please check availability of the product with your local sales representative or your local customer service.

This product contains no detectable latex.



Dilation

CRE™ CONTROLLED RADIAL EXPANSION DILATION BALLOONS (CONTINUED)

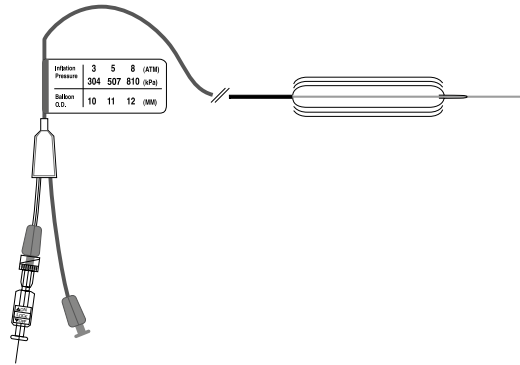

CRE™ Wire-guided Esophageal/Pyloric Dilation Balloons



Order Number	Inflated O.D. (mm)	Balloon Length (cm)	Inflation Pressure		Minimum Working Channel (mm)	Catheter Diameter (F) / (mm)	Working Length (cm)
			(ATM)	(kPa)			
M00558390	6-7-8	5.5	3-6-10	304-608-1013	2.8	7.5 / 2.50	180
M00558400	8-9-10	5.5	3-5.5-9	304-557-912	2.8	7.5 / 2.50	180
M00558410	10-11-12	5.5	3-5-8	304-507-810	2.8	7.5 / 2.50	180
M00558420	12-13.5-15	5.5	3-4.5-8	304-456-810	2.8	7.5 / 2.50	180
M00558430	15-16.5-18	5.5	3-4.5-7	304-456-709	2.8/3.2*	7.5 / 2.50	180
M00558440**	18-19-20	5.5	3-4.5-6	304-456-608	2.8/3.2*	7.5 / 2.50	180

Packaged one per box


Recommended Inflation Device: Alliance II Integrated Inflation System Re-usable Handle M00550620, Sterile Syringe M00550601

Pre-assembled .035in (0.89mm) Guidewire

* Requires a 2.8mm Olympus Endoscope channel or a 3.2mm Pentax or Fujinon Endoscope channel for alimentary tract.

** Esophageal application only.

This product contains no detectable latex.

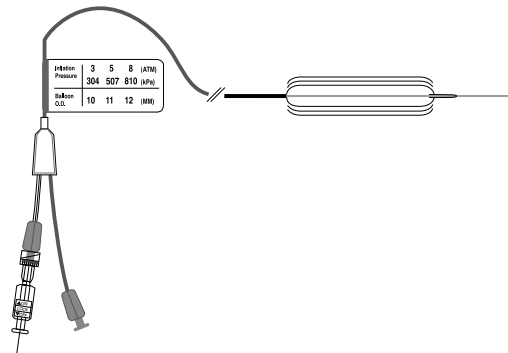

CRE™ Wire-guided Esophageal/Pyloric/Colonic Dilation Balloons



Order Number	Inflated O.D. (mm)	Balloon Length (cm)	Inflation Pressure		Minimum Working Channel (mm)	Catheter Diameter (F) / (mm)	Working Length (cm)
			(ATM)	(kPa)			
M00558450	6-7-8	5.5	3-6-10	304-608-1013	2.8/3.2*	7.5 / 2.50	240
M00558460	8-9-10	5.5	3-5.5-9	304-557-912	2.8/3.2*	7.5 / 2.50	240
M00558470	10-11-12	5.5	3-5-8	304-507-810	2.8/3.2*	7.5 / 2.50	240
M00558480	12-13.5-15	5.5	3-4.5-8	304-456-810	2.8/3.2*	7.5 / 2.50	240
M00558490	15-16.5-18	5.5	3-4.5-7	304-456-709	2.8/3.2*	7.5 / 2.50	240
M00558500**	18-19-20	5.5	3-4.5-6	304-456-608	2.8/3.2*	7.5 / 2.50	240

Packaged one per box


Recommended Inflation Device: Alliance II Integrated Inflation System Re-usable Handle M00550620, Sterile Syringe M00550601

Pre-assembled .035in (0.89mm) Guidewire

* Requires a 2.8mm Olympus Endoscope channel or a 3.2mm Pentax or Fujinon Endoscope channel for alimentary tract.


** Esophageal or Colonic application only.

This product contains no detectable latex.



Dilation

CRE™ CONTROLLED RADIAL EXPANSION DILATION BALLOONS (CONTINUED)

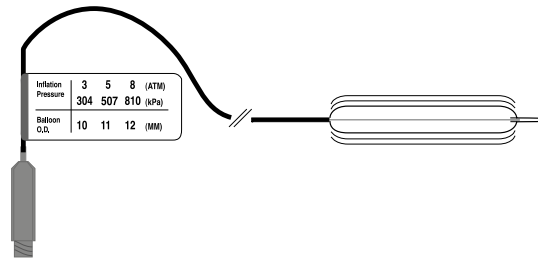

CRE™ Fixed Wire Dilation Balloons




Order Number	Inflated O.D. (mm)	Balloon Length (cm)	Inflation Pressure (ATM) (kPa)		Minimum Working Channel (mm)	Catheter Diameter (F) / (mm)	Working Length (cm)
M00558330	6-7-8	8	3-6-10	304-608-1013	2.8	6 / 2.00	180
M00558340	8-9-10	8	3-5.5-9	304-557-912	2.8	6 / 2.00	180
M00558350	10-11-12	8	3-5-8	304-507-810	2.8	6 / 2.00	180
M00558360	12-13.5-15	8	3-4.5-8	304-456-810	2.8	6 / 2.00	180
M00558370	15-16.5-18	8	3-4.5-7	304-456-709	2.8	6 / 2.00	180
M00558380	18-19-20	8	3-4.5-6	304-456-608	2.8	6 / 2.00	180

Packaged one per box


Recommended Inflation Device: Alliance™ II Integrated Inflation System Re-usable Handle M00550620, Sterile Syringe M00550601

This product contains no detectable latex.



Dilation

MAX FORCE™ TTS DILATION BALLOONS

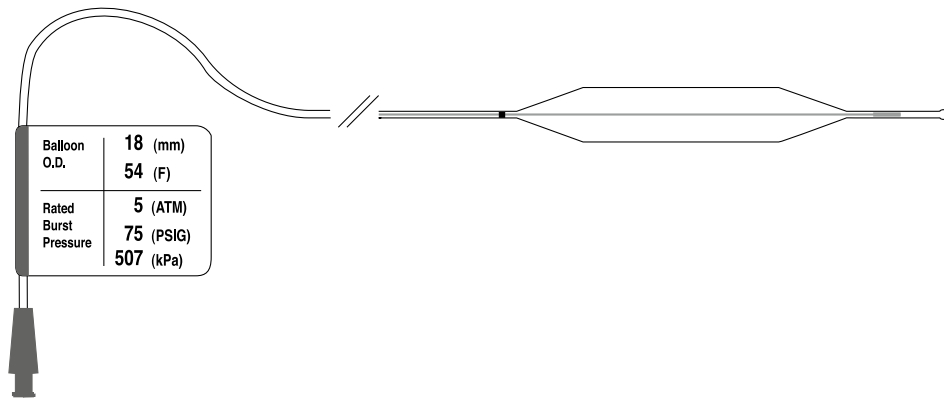

Max Force™ TTS Esophageal Dilation Balloons



Order Number	Inflated O.D. (mm)	Balloon Length (cm)	Inflation Pressure		Minimum Working Channel (mm)	Catheter Diameter (F) / (mm)	Working Length (cm)
			(ATM)	(kPa)			
M00589060	6	6	10	1013	2.8	6 / 2.00	180
M00589080	8	6	10	1013	2.8	6 / 2.00	180
M00589100	10	6	7	709	2.8	6 / 2.00	180
M00589120	12	6	7	709	2.8	6 / 2.00	180
M00589140	14	6	7	709	2.8	6 / 2.00	180
M00589150	15	6	5	507	2.8	6 / 2.00	180
M00589160	16	6	5	507	2.8	6 / 2.00	180
M00589180	18	6	5	507	2.8	6 / 2.00	180

Packaged one per box

Recommended Inflation Device: Alliance™ II Integrated Inflation System Re-usable Handle M00550620, Sterile Syringe M00550601

This product contains no detectable latex.

Rigiflex™ II Achalasia Dilation Balloons*




Order Number	Inflated O.D. (mm)	Balloon Length (cm)	Catheter Diameter (F) / (mm)	Working Length (cm)	Recommended Guidewire (in) / (mm)**
M00554500	30	10	14 / 4.67	90	.038 / 0.97
M00554510	35	10	14 / 4.67	90	.038 / 0.97
M00554520	40	10	14 / 4.67	90	.038 / 0.97

Packaged one per box

* Product shipped sterile. Recommended use with Achalasia Pneumatic Hand Pump and Monitor, M00553200


** Guidewire included with Rigiflex™ II Balloon Dilation Catheter

This product contains no detectable latex.



Dilation

INFLATION SYSTEMS

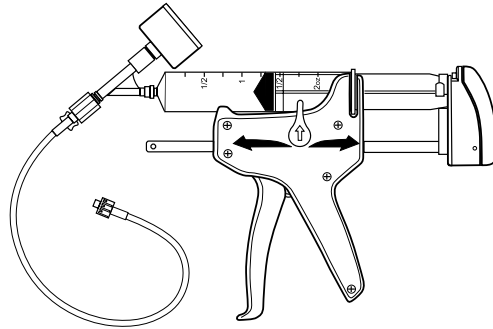

Alliance™ II Inflation System

Order Number	Description	Units
M00550620	Alliance™ II Inflation Handle	box 1
M00550601	⊗ 60ml Syringe/Gauge Assembly	box 5

DILATION ACCESSORIES

Inflation/Deflation Devices and Accessories

Order Number	Description	Units
M00553200	Achalasia Pneumatic Inflator and Monitor	box 1

RX Biliary Dilation Balloons are located in the RX Biliary Section on page 6

Biliary Dilation Balloons are located in the Biliary Section on page 13

Pulmonary Dilation Balloons are located in the Pulmonary Section on page 75